

# Chikungunya NS1 Antigen Rapid Test Kit (Colloidal Gold)



## Instruction for Use

Read this instruction carefully before use

A rapid test for the qualitative detection of Human Chikungunya virus NS1 antigen in human serum, plasma or whole blood. For professional medical institutions use only, Not for self testing.

### PRODUCT NAME

Chikungunya NS1 Antigen Rapid Test Kit (Colloidal Gold)

### SPECIFICATION

25 tests/kit; 5 tests/kit; 1 test/kit

### INTENDED USE

The Chikungunya NS1 Rapid Test is a lateral flow chromatographic immunoassay for the qualitative detection of Chikungunya virus antigen (Chikungunya Ag) in human serum, plasma or whole blood. It is intended to be used as a screening test and as an aid in the diagnosis of infection with Chikungunya viruses. Any reactive specimen with the Chikungunya Ag Rapid Test must be confirmed with alternative testing method(s) and clinical findings.


### SUMMARY AND EXPLANATION THE TEST

Chikungunya is a rare viral infection transmitted by the bite of an infected Aedes aegypti mosquito. It is characterized by a rash, fever, and severe joint pain (arthralgias) that usually lasts for three to seven days. The name is derived from the Makonde word meaning "that which bends up" in reference to the stooped posture developed as a result of the arthritic symptoms of the disease. It occurs during the rainy season in tropical areas of the world, primarily in Africa, South-East Asia, southern India and Pakistan. The symptoms are most often clinically indistinguishable from those observed in dengue fever. Indeed, dual infection of dengue and chikungunya has been reported in India. Unlike dengue, hemorrhagic manifestations are relatively rare and most often the disease is a self limiting febrile illness. Therefore it is very important to clinically distinguish dengue from CHIK infection. CHIK is diagnosed based on serological analysis and viral isolation in mice or tissue culture. An IgM immunoassay is the most practical lab test method. The Chikungunya IgG/IgM Rapid Test utilizes recombinant antigens derived from its structure protein, it detects IgG/IgM anti-CHIK in patient serum or plasma within 20 minutes. The test can be performed by untrained or minimally skilled personnel, without cumbersome laboratory equipment.

### PRINCIPLE

The Chikungunya NS1 Rapid Test is a lateral flow chromatographic immunoassay. The test cassette consists of: 1) a burgundy colored conjugate pad containing mouse anti-Chikungunya NS1 antigen conjugated with colloidal gold (Chikungunya Ab conjugates), 2) a nitrocellulose membrane strip containing a test band (T band) and a control band (C band). The T band is pre-coated with rabbit anti-Chikungunya NS1 antigen, and the C band is pre-coated with goat anti-mouse IgG antibody. The antibodies to Chikungunya antigen recognize the antigens.

When an adequate volume of test specimen is dispensed into the sample well of the cassette, the specimen migrates by capillary action across the test cassette. Chikungunya NS1 Ag if present in the specimen will bind to the Chikungunya Ab conjugates. The immunocomplex is then captured on the membrane by the pre-coated rabbit anti-Chikungunya NS1 antibody, forming a burgundy colored T band, indicating Chikungunya Ag positive test result.



Absence of the T band suggests a negative result. The test contains an internal control

(C band) which should exhibit a burgundy colored band of the immunocomplex of goat anti-mouse IgG/mouse IgG-gold conjugate regardless of the presence of colored T band. Otherwise, the test result is invalid and the specimen must be retested with another device.

### REAGENTS AND MATERIALS PROVIDED

Components	25tests/kit	5tests/kit	1test/kit
Cassettes	25 cassettes with dependent sealed foil pouch	5 cassettes with dependent sealed foil pouch	1 cassette with dependent sealed foil pouch
Sample Diluent Solution with dropper	25tubes (300ul/tube)	5tubes (300ul/tube)	300ul/tube
Transfer tube	25 pcs	5 pcs	1 pcs
Package insert	1	1	1

### MATERIALS REQUIRED BUT NOT PROVIDED

Clock or Timer

### WARNINGS AND PRECAUTIONS

For in Vitro Diagnostic Use

- 1.This package insert must be read completely before performing the test. Failure to follow the insert gives inaccurate test results.
- 2.Do not open the sealed pouch, unless ready to conduct the assay.
- 3.Do not use expired devices.
- 4.Bring all reagents to room temperature (15°C-30°C) before use.
- 5.Do not use the components in any other type of test kit as a substitute for the components in this kit.
- 6.Do not use hemolyzed blood specimen for testing.
- 7.Wear protective clothing and disposable gloves while handling the kit reagents and clinical specimens. Wash hands thoroughly after performing the test.
- 8.Users of this test should follow the US CDC Universal Precautions for prevention of transmission of HIV, HBV and other blood-borne pathogens.
- 9.Do not smoke, drink, or eat in areas where specimens or kit reagents are being handled.
- 10.Dispose of all specimens and materials used to perform the test as biohazardous waste.
- 11.Handle the Negative and Positive Control in the same manner as patient specimens.
- 12.The testing results should be read within 25 minutes after a specimen is applied to the sample well or sample pad of the device. Read result after 25 minutes may give erroneous results.
- 13.Do not perform the test in a room with strong air flow, ie. electric fan or strong air-conditioning.

### REAGENT PREPARATION AND STORAGE INSTRUCTIONS

All reagents are ready to use as supplied. Store unused test device unopened at 2°C-30°C. The positive and negative controls should be kept at 2°C-8°C. If stored at 2°C-8°C, ensure that the test device is brought to room temperature before opening. The test device is stable through the expiration date printed on the sealed pouch. Do not freeze the kit or expose the kit over 30°C.

### SPECIMEN COLLECTION AND HANDLING

Consider any materials of human origin as infectious and handle them using standard bio-safety procedures.

#### Plasma

- 1.Collect blood specimen into a lavender, blue or green top collection tube (containing EDTA, citrate or heparin, respectively in Vacutainer®) by veinpuncture.
- 2.Separate the plasma by centrifugation.
- 3.Carefully withdraw the plasma into new pre-labeled tube.

#### Serum

- 1.Collect blood specimen into a red top collection tube (containing no anticoagulants in Vacutainer®) by veinpuncture.
- 2.Allow the blood to clot.
- 3.Separate the serum by centrifugation.
- 4.Carefully withdraw the serum into a new pre-labeled tube.
- 5.Test specimens as soon as possible after collecting. Store specimens at 2°C to 8°C if not tested immediately.
- 6.Store specimens at 2°C to 8°C up to 5 days. The specimens should be frozen at

-20°C for longer storage


#### Blood

Drops of whole blood can be obtained by either finger tip puncture or veinpuncture. Do not use any hemolyzed blood for testing. Whole blood specimens should be stored in refrigeration (2°C-8°C) if not tested immediately. The specimens must be tested within 24 hours of collection. Avoid multiple freeze-thaw cycles. Prior to testing, bring frozen specimens to room temperature slowly and mix gently. Specimens containing visible particulate matter should be clarified by centrifugation before testing.

### ASSAY PROCEDURE


- Step 1: Bring the specimen and test components to room temperature if refrigerated or frozen. Once thawed, mix the specimen well prior to assay.
- Step 2: When ready to test, open the pouch at the notch and remove device. Place the test device on a clean, flat surface.
- Step 3: Be sure to label the device with specimen's ID number.
- Step 4: **For whole blood test**

- Apply 1 drop of whole blood (about 20 µL) into the sample well.
- Then add 2 drops (about 60-70 µL) of Sample Diluent immediately.

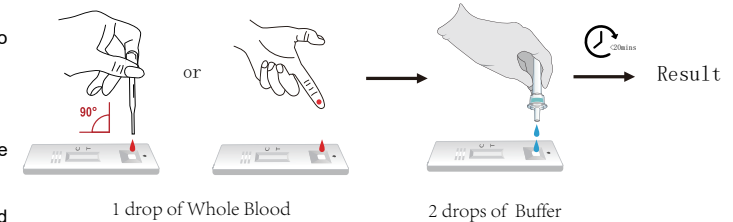

#### For serum or plasma test

- Fill the pipette dropper with the specimen.
- Holding the dropper vertically, dispense 1 drop (about 30-35 µL) of specimen into the sample well making sure that there are no air bubbles.
- Then add 2 drops (about 60-70 µL) of Sample Diluent immediately.

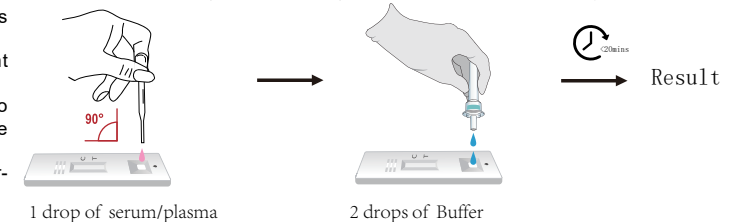

Step 5: Set up timer.

Step 6: Results can be read in 20 minutes. Positive results can be visible in as short as 1 minute.

**Don't read results after 30 minutes. To avoid confusion, discard the test device after interpreting the result.**

### QUALITY CONTROL

Internal Control: This test contains a built-in control feature, the C band. The C line develops after adding specimen and sample diluent. Otherwise, review the whole procedure and repeat test with a new device.


External Control: Good Laboratory Practice recommends using the external controls, positive and negative, to assure the proper performing of the assay, in particularly, under the following circumstances:

- a. New operator uses the kit, prior to performing testing of specimens.
- b. A new lot of test kit is used.
- c. A new shipment of kits is used.
- d. The temperature used during storage of the kit fall outside of 2°C -30°C .
- e. The temperature of the test area falls outside of 15°C -30°C .

### Negative Control

Only the C band shows color development. The T band shows no color development.

### Positive Control




Both C and T bands show color development. The appearance of any burgundy color in the T band, regardless of intensity, must be considered as presence of the band.



### INTERPRETATION OF ASSAY RESULT


**1. NEGATIVE RESULT:** If only the C band is developed, the test indicates that the level of Chikungunya Ag in the specimen is undetectable. The result is negative or non-reactive.



**2. POSITIVE RESULT:** If both C and T bands are developed, the test indicates that the specimen contains Chikungunya Ag. The result is positive or reactive. Samples with positive results should be confirmed with alternative testing method(s) such as PCR or ELISA and clinical findings before a positive determination is made.



**3. INVALID:** If no C band is developed, the assay is invalid regardless of color development on the T band as indicated below. Repeat the assay with a new device.

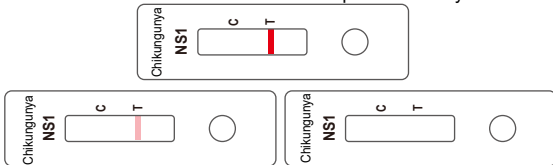

### PERFORMANCE CHARACTERISTICS

#### Clinical Performance

A total of 654 patient samples from susceptible subjects were tested by the Chikungunya NS1 Rapid Test and by a commercial EIA. Comparison for all subjects is showed in the following table:

Chikungunya NS1 EIA Test	Chikungunya NS1 Rapid Test		
	Positive	Negative	Total
Positive	289	5	294
Negative	3	381	384
<b>Total</b>	<b>292</b>	<b>386</b>	<b>678</b>

Relative Sensitivity: 98.30%, Relative Specificity: 99.22%, Overall Agreement: 98.82%.

#### LIMITATIONS OF TEST

- The Assay Procedure and the Assay Result Interpretation must be followed closely when testing the presence of Chikungunya Ag in serum, plasma or whole blood, from individual subjects. Failure to follow the procedure may give inaccurate results.
- The Chikungunya NS1 Rapid Test is limited to the qualitative detection of Chikungunya Ag in human serum, plasma or whole blood. The intensity of the test band does not linearly correlate with Chikungunya Ag titer of the specimen.
- A negative test result does not preclude the possibility of exposure to or infection with Chikungunya viruses.
- A negative result can occur if the quantity of Chikungunya Ag present in the specimen is below the detection limits of the assay, or the dengue Ag that are detected

are not present during the stage of disease in which a sample is collected.

5. Some specimens containing unusually high titer of heterophile antibodies or rheumatoid factor may affect expected results.

6. If the symptom persists, while the result from Chikungunya NS1 Rapid Test is negative or non-reactive result, it is recommended to re-sample the patient few days late or test with an alternative test device such as PCR, ELISA.

7. The results obtained with this test should only be interpreted in conjunction with other diagnostic procedures and clinical findings.

### SYMBOLS

Symbol	Used For	Symbol	Used For
	Use-by date		Consult instructions for use
	Batch code		In vitro diagnostic medical device
	Temperature limit		Manufacturer
	Please don't reuse it		Keep away from sunlight
	Don't use the product when the package is damaged		Keep dry
	Date of manufacture		Tests per kit
	CE Mark		Biological Risks
	Authorized representative in the European Community		

### BASIC INFORMATION



**Ningbo BESTest Bio-technology Co.,Ltd.**

Address: No.80 building, No.777, Qing Feng Road, Cicheng Town, Jiangbei District, Ning Bo, Zhejiang, China 315033  
Tel: 0086 571 2799 8736



**SUNGO Europe B.V.**

Address: Olympisch Stadion 24, 1076DE Amsterdam, Netherlands.